

Measurement file : 20171109-01.dat

Template file : Rn222 direct extraction.par

Valid Assay


Measurement date : 2017-11-09

Measurement time : 10:14:04

Table arranged data

SID	Collect Date	Vol (L)	Water/Cocktail	CPMB	DPMB	pCi/L-B	CPMA	DPMA	pCi/L-A
Blank	11/9/2017 8:05:00 AM	0.010	1.00	79	0	0	1	0	0
Std1	11/9/2017 8:05:00 AM	0.010	1.00	1850	1927	86806	2249	2284	41828

Spectra Graphics

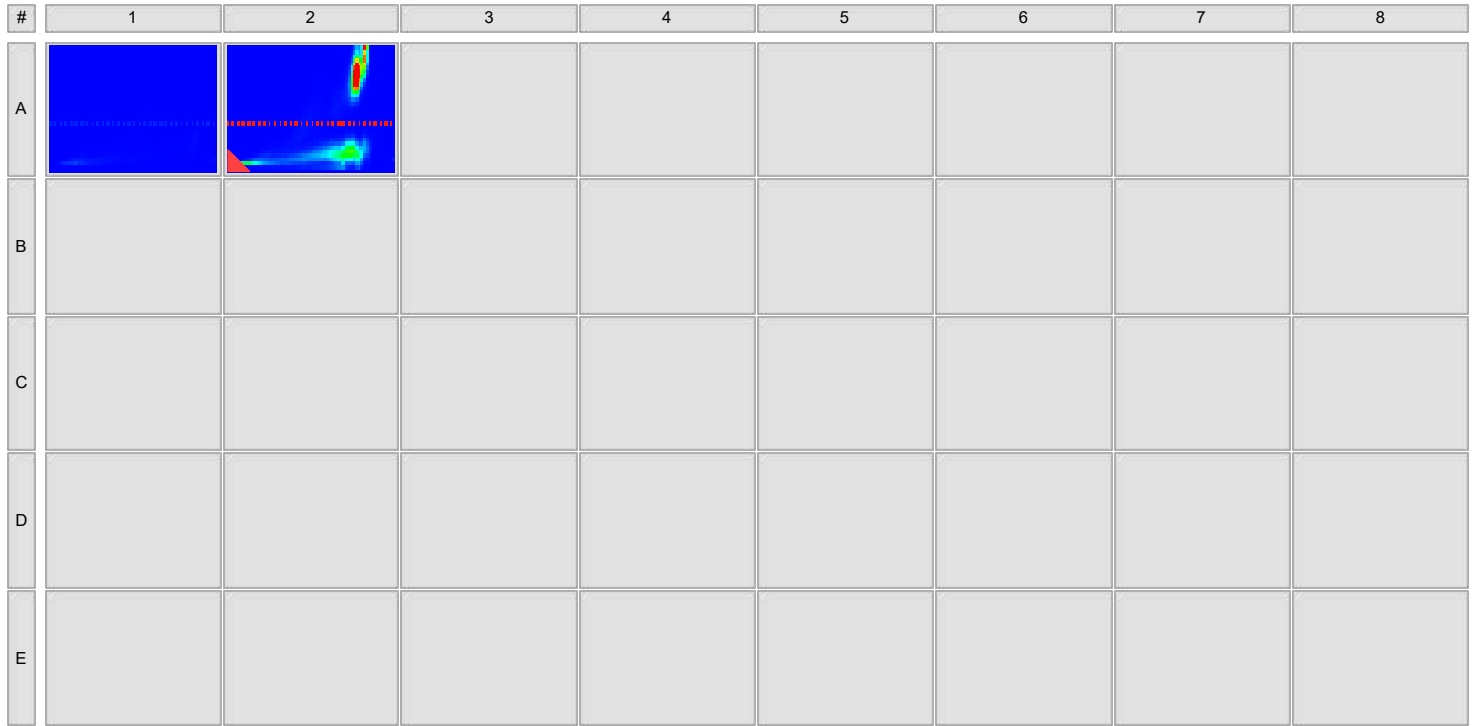

Spectra Graphics

